

# PRV

PATENT- OCH REGISTRERINGSVERKET  
Patentavdelningen

10532790  
DT01 Rec'd PCT/PTC 25 APR 2005

## Intyg Certificate

*Härmed intygas att bifogade kopior överensstämmer med de handlingar som ursprungligen ingivits till Patent- och registreringsverket i nedannämnda ansökan.*

*This is to certify that the annexed is a true copy of the documents as originally filed with the Patent- and Registration Office in connection with the following patent application.*



(71) Sökande St Jude Medical AB, Järfälla SE  
Applicant (s)

(21) Patentansökningsnummer 0203220-9  
Patent application number

(86) Ingivningsdatum 2002-10-31  
Date of filing

Stockholm, 2003-06-02

För Patent- och registreringsverket  
For the Patent- and Registration Office

Hjordis Segerlund

Avgift  
Fee 170:-

**Motion sensor**

Technical field

5 The invention concerns a motion sensor for measuring a patient's activity level comprising a fluid-tight, bio-compatible housing, a plurality of electrodes being coupled to the housing and the housing comprising a fluid. Furthermore, the invention relates to an implantable medical device, such as a heart stimulator, e.g. cardiac pacemaker comprising the motion sensor.

10

Prior art

Heart stimulators, below exemplified by pacemakers are used to e.g. pace the frequency of the heart. They have been of greatest importance for helping individuals suffering from various heart diseases and/or failures to live rather normal lives.

15 Pacemakers function by generating electrical pulses, which stimulate the heart. In order to pace the heart in a correct way, the specific pulse pattern of the individual heart must be known. External parameters, such as the motion of the patient, are advantageously known, in order for the pacemaker to stimulate the heart as correctly as possible.

20

Normally, the motion of the patient is measured by some kind of motion sensor, which sensor is connected to the pacemaker. US-A-5755741 discloses an implantable sensor providing an indication of movement and orientation of a patient.

25

The sensor may be connected to a pacemaker. The sensor comprises a cylindrical enclosure having a central electrode within a cavity of the enclosure, and one or more peripheral electrodes within the cavity. An electrolytic fluid is positioned in the enclosure so that movement of the sensor results in variations of the amount of the fluid between the central electrode and one or more of the peripheral electrodes.

An alternating current applied to the electrodes will render a voltage signal, which varies in accordance with the movements of the fluid (and the sensor).

5 US-A-5833713 discloses an accelerometer-based, multi-axis physical activity sensor for use with a rate-responsive pacemaker. A piezoelectric polymer film is adhered to the surface of an electrically conductive substrate on the sensor. In response to bodily accelerations the piezoelectric film produces an output signal.

10 US-A-5233984 discloses a multi-axis sensor, for example connected to a pacemaker, for measuring a patient's activity level. The sensor comprises a hermetically sealed, fluid-tight, biocompatible housing, whereby a plurality of electrodes is coupled to the sides of the housing, and a central electrode is positioned within the housing. An electrically conductive electrolyte fills about half of the housing, allowing voltage changes, due to motion of the sensor, between the central electrode  
15 and the other electrodes to be monitored.

Also, US-A-4869251 discloses a pacemaker having a sensor for detecting inertial and/or rotational movements of a patient. The sensor has a hollow member, with at least one freely moveable member therein generating a mechanical vibration upon  
20 movement of the patient. A transducer generates an electric signal corresponding to the mechanical vibrations. It is stated that the hollow member may be filled with a fluid and/or a plurality of particles producing pressure to the walls of the hollow member. It is also stated that the sensitivity of the sensor may be different in different directions. For example, the moveable element may be a magnetic dipole, and  
25 the transducer may be one or more coils arranged around the hollow member, whereby a current is generated in the coils when the moveable element changes position in the interior of the hollow member. Depending on configuration, the mobility of the movable element may however degrade due to mechanical wear.

Accordingly, the motion sensors of the prior art normally rely on moving mechanical components, and therefore they may be difficult to miniaturise further. This is a problem, since the size of the motion sensor (and pacemakers) advantageously is as small as possible, in order to disturb the biological system into which they are put as little as possible. Furthermore, as mentioned above, mechanically based sensors may suffer from mechanical wear, which can lead to their failure.

Accordingly, it is an object of the present invention to provide a motion sensor, which overcomes the drawbacks of the prior art, and thereby comprises as few mechanical parts as possible, the sensor further being as small as possible, and relying on a technical principle making it as resistant to failure as possible.

#### Summary of the invention

These and other objects are accomplished by a motion sensor according to claim 1 of the present invention, which relies on the principle of an electrically detectable anisotropic fluid, which fluid orients itself in relation to external motion.

Hereby, a sensor is provided in which no moving parts are comprised, and which therefore is possible to make very small.

In a preferred embodiment, the anisotropic fluid comprises long rigid LCP-molecules, on which electrically detectable magnetic nanoparticles are covalently linked.

In another embodiment a magnetic field is applied to the anisotropic fluid, and the alignment of the anisotropic molecules is detected by measuring the capacitance of the fluid.

Moreover, the invention relates to an electrically detectable anisotropic fluid comprising a liquid crystalline polymer (LCP) as the anisotropic fluid, which LCP is covalently bound to an iron-oxide nanoparticle. This fluid is specifically suitable for use in the motion sensor of the invention.

5

Furthermore, the invention relates to an implantable pacemaker comprising the motion sensor of the invention. Hereby, a patient's heart is paced as a response to the patient's motion, as sensed by the motion sensor of the invention.

10 Accordingly, the drawbacks of the prior art are overcome.

#### Short description of the drawings

15 Figure 1 shows a principal sketch of a motion sensor according to one embodiment of the invention.

Figure 2 shows a principal coupling scheme for a motion sensor of the invention coupled to a rate response pacemaker.

20 

#### Preferred embodiments

25 The idea of the invention is to provide a motion sensor, especially adapted for use with a pacemaker, which is as small as possible, and which circumvents the problem of mechanical wear in a sensor comprising several mechanical parts. This is provided by a sensor, which relies on the principle of an anisotropic fluid or an anisotropic molecule within a fluid. Thereby, the only moving parts of the sensor are fluids.

30 Accordingly, in a first aspect the invention relates to a motion sensor for measuring a patient's activity level comprising a fluid-tight, bio-compatible housing, a plurality

of electrodes being coupled to the housing, the housing comprising a fluid that comprises at least one anisotropic molecule, the anisotropic properties of which are changed in relation to the motion of the fluid, whereby the state of the anisotropic molecules of the fluid is detectable by the electrodes.

5

In a preferred embodiment, the motion sensor is implantable in the patient in question. However, the motion sensor may also be adapted for external use, i.e. not being implanted in the body of the patient, but communicating by for example some telemetric means with an implanted pacemaker.

10

By a "patient" is in the context of the invention meant an animal, especially a human, which is in need of a motion sensor. This may for example include persons which have a pacemaker or whom is to be equipped with a pacemaker. However, the motion sensor of the invention must not necessarily be coupled to a pacemaker, but may also be connected to any other device or circuitry for which the output of the motion sensor is relevant.

15

By a patient's "activity level" is meant the degree of motion for the specific patient. For example, for a pacemaker to deliver the correct pulses to a patients heart, it is important to correlate these pulses with the "activity level" of the patient, in order for the pacing pulses and the resulting heart responses to be suited for the patients present need. Thus, it is preferred that the paced heart rate is adaptable to different levels of exertion by the patient.

20

By "a plurality of electrodes " is meant at least one electrode pair, having the capacity to monitor at least one electronic parameter.

25

An anisotropic molecule will orient itself in relation to the motional stress it is subjected to. Thus, for example, an anisotropic molecule may exhibit anisotropic properties at rest and isotropic properties when agitated (i.e. different states). Accord-

30

ingly, a plurality of molecules of this kind will, like a crystal, align in a common direction at rest, or in a laminar shearing force. The viscosity, as well as several other physico-chemical properties, such as optical transmission, heat transfer, polarity, conductivity etc., will then be very different in the alignment direction compared to other directions, especially the perpendicular direction. However, if agitated, the molecular alignments will become randomised, and as a result properties such as viscosity or dielectric constant will be practically equal in all directions. Thus, when a patient carrying the sensor of the invention moves, the sensor will sense these movements (or lack of movements) and create an output signal, which is based on them.

Liquid crystalline polymers (LCP's)(Langmuir 2001, 17, 2900-2906) are fluids having anisotropic properties at rest and isotropic properties during agitation. LCP's, in the context of the invention, are long rigid molecules, which have an aspect-ratio (length/diameter) of greater than about (10/1). One example, which is suitable for the purposes of the invention, is poly-(p-phenylene) with a degree of polymerisation (n) equal to or greater than 10. In this context, the aspect-ratio would be a more relevant term than for example molecule length, since a rigid rod polymer with a wide diameter will not exhibit anisotropic properties at the same length or degree of polymerisation as a rigid rod polymer with a narrow diameter. The aspect-ratio, however, provides a good way to measure the intrinsic anisotropy of the polymer molecules.

Thus, according to one embodiment of the invention the anisotropic molecule is a liquid crystalline polymer (LCP).

Some other examples of liquid crystalline polymers suitable for the invention are given below. However, this list is not exhaustive, and other compounds may also be used.

A copolymer of p-hydroxybenzoic acid and polyethylene terephthalate. (Japanese Patent Publication No. 18016/1981); a copolymer of p-hydroxybenzoic acid, polyethylene terephthalate, aromatic diol (such as 4,4'-dihydroxybiphenyl), and aromatic dicarboxylic acid, with improved flowability and heat resistance. (Japanese Patent Laid-open No. 30523/1988); a copolymer of p-hydroxybenzoic acid, 4,4'-dihydroxybiphenyl, t-butylhydroquinone, and terephthalic acid. (Japanese Patent Laid-open No. 164719/1987); a copolymer of p-hydroxybenzoic acid, 4,4'-dihydroxybiphenyl, isophthalic acid, and terephthalic acid. (Japanese Patent Publication No. 24407/1982 and Japanese Patent Laid-open No. 25046/1985); a copolymer of p-hydroxybenzoic acid and 6-hydroxy-2-naphthoic acid. (Japanese Patent Laid-open No. 77691/1979); copolyesters of terephthalic acid, alkylhydroquinone, p-hydroxybenzoic acid and poly(alkylene terephthalate), the alkylene substituent preferably comprising ethylene or butylene and the alkyl substituent of the hydroquinone preferably comprising a lower alkyl group such as propyl or (tertiary) butyl; copolyesters of p-hydroxybenzoic acid and poly(alkylene terephthalate), the alkylene group preferably being ethylene or butylene; copolyesters of terephthalic acid, alkylhydroquinone, p-hydroxybenzoic acid and hydroxyalkylphenyl-alkanoic acids, the alkyl-substituent of the hydroquinone preferably comprising a lower alkyl group such as propyl or (tertiary) butyl, the alkanoic acid preferably containing 3 to 8 carbon atoms, propanoic acid being particularly preferred, and blockcopolyesters of trimellithic imide-terminated poly(THF) or polysilicone, containing the imide group in para- or meta-position i.e. N-(4-carboxy-phenyl)-trimellit imide or N-(3'-acetoxy-phenyl)-trimellit imide, with acetoxybenzoic acid and at least one repeating unit selected from the group comprising diacetoxy diphenyl, hydroquinone diacetate, terephthalic acid, a trimer designated HBA--HQ--HBA (the synthesis of which is described in Europ. Polym. J. 20, 3, 225-235 (1984), and poly(ethylene terephthalate) (PET).

The molecular weight of the liquid crystal polymer used in the present invention depends on the character of the repeating units of the LCP. Usually, the molecular



weight is in the range of about 1,000 to 300,000. If fully aromatic polyesters are used as LCP's, their molecular weight is typically in the range of about 2,000 to 200,000, preferably about 10,000 to 50,000.

5 More general details on liquid crystalline polymers and their properties and applications are given in an article titled "Liquid Crystal Polymers and Their Applications" by Chung et al. in Handbook of Polymer Science and Technology, Vol. 2 (1989) 625-675.

10 In order to be able to detect the anisotropic properties one may for example attach a doping agent to the anisotropic molecule, which doping agent have the capacity to provide a readable electronic signal. Thus, the doping agent constitutes an electrically detectable part. Hereby, a patient's activity level is possible to monitor.

15 The doping agent is coupled to the LCP-molecule by any common chemical bonding technique. Preferably, the doping agent is coupled to the LCP-molecule by covalent bonding. The skilled person in the art easily recognises techniques for binding the doping agent to the LCP, e.g. by hydrosilylation reactions using organosilane intermediates, for example dimethylvinyl silane.

20 Therefore, according to another embodiment the anisotropic molecule comprises an electrically detectable part.

25 The production of silica-coated iron oxide nanoparticles is described in the reference article Langmuir, Vol 17, No. 10, 2001 (2900-2906). Basically, they are produced in solution from appropriate chemical reagents, aided by suspension in organic surfactants. The particles are treated with tetraethylorthosilicate (TEOS) to form a silica coating. These particles are magnetic, and can be bound to an isotropic (rigid rod) molecule using covalent bonding and standard silica surface treatment chemistry, for example by silanization with dimethylvinyl silane. In one embodiment

30

of the present invention, the silane group bonds to the silica surface, and the vinyl group can form a covalent bond with many different kinds of organic molecules, including Liquid Crystalline Polymers (LCP's) containing dipoles. Under a small magnetic field (B), such as greater than about 0.5 Gauss, a preferential orientation will be induced, so that the magnetic particles line up in the magnetic field. The degree of alignment is preferably detected by measurement of capacitance across the fluid. The tendency for alignment is dependent on agitation because the dipoles will be forced by the magnetic particles to line up in the preferential orientation, but that orientation is disturbed by fluid motion.

For a principal sketch of one embodiment of the motion sensor of the invention see figure 1. The sensor 10 comprises a housing 11, which is filled by a fluid. The fluid comprises at least partly anisotropic molecules of the invention. Furthermore, a magnetic field is generated by the magnets 14 and 15. A capacitor 12 and 13 measures the capacitance of the fluid, and thus a variation in the anisotropic status of the fluid is monitored.

Examples of doping agents are ions or molecular dipoles. Preferably, a magnetically aligned nanoparticle (Langmuir 2001, 17, 2900-2906), or a charge-separated ion-pair, such as a zwitterionic pair (positive charge at one end, negative at the other) is used. The nanoparticle is in a preferred embodiment an iron-oxide nanoparticle, wherein iron-oxide may be represented by e.g.  $\text{Fe}_3\text{O}_4$ , or  $\gamma\text{-Fe}_2\text{O}_3$  (Langmuir 2001, 17, 2900-2906)

Thus, in yet another embodiment of the invention the detectable part is a magnetic nanoparticle, a zwitterionic pair or a charge separated ion-pair, preferably a magnetic iron-oxide nanoparticle.

Hereby, the electrical/magnetic signature is representative of the degree of alignment of the LCP's. As a consequence, the amount of agitation (i.e. patient activity)

is correlated to the electrical or magnetic signal, which the sensor and/or pacemaker circuitry is designed to detect. As a result a motion sensor having no moving parts (except the anisotropic fluid) and that can be made very small can be manufactured. For example, the sensor may have a cavity volume of a few mm<sup>3</sup> or less, such as less than 10 mm<sup>3</sup>, preferably less than 5 mm<sup>3</sup>, most preferably less than 1 mm<sup>3</sup>.

The suitable electronic signal to be monitored may vary depending on the nature of the system and its chemical content. However, for many applications measure of capacitance is suitable. In other cases measurement of voltage, voltage changes, impedance or resistance may be suitable.

Thus, in still another embodiment the state of the anisotropic molecule is monitored by measuring the capacitance in the fluid.

In yet another embodiment the state of the anisotropic molecule is monitored by measuring the resistance in the fluid.

In yet another embodiment, coils are arranged around the housing. Upon a variation in the state of the anisotropic fluid, a voltage is induced in the coils, which voltage is used as a signal. For example, the coil may be of insulated silver/copper wire.

The nanoparticulate size of the anisotropic entity molecules enables low enough viscosity that no moving parts (other than fluid) is necessary, even in small devices like a pacemaker. A half-empty cylinder is one preferred example of the container.

This container preferably has a magnetic N and a magnetic S pole provided by placement of permanent magnets 14 and 15 on opposite sides of its diameter. The electric sensor (e.g. capacitor electrodes 12 and 13) may also be on opposite sides of the cylinder diameter, though preferably normal (90 degrees) to the magnetic diameter (see figure 1).

It is not required to have the capacitor electrodes normal to the magnetic field, but it provides the optimum signal output. Each molecule of the fluid will act as a dipole with a dipole moment in a particular direction. When in a magnetic field, the dipole moments will tend to align in due to being bound to the magnetic particles as described in the reference article. The net dipole moment of the fluid is then finite and detectable as capacitance between the capacitance electrode. This "high order state" is detectable across any plane of the fluid except that parallel to the magnetic field, since in the parallel plane the LCP molecule ends face the electrodes and the LCP fluid would appear to the sensor to be small molecules with no preferable orientation in that plane. Therefore, in the "high order state", the signal is obtained as long as the capacitor electrodes are not in the parallel plane, a detectable signal in any other plane, and an optimum signal is obtained in the perpendicular plane. Note that when agitated, the dipoles become randomly oriented yielding a much lower net dipole moment - this "low order state" gives the same signal output independent of orientation between the capacitor electrodes and the magnetic field. So to achieve the maximum difference between the "at rest" state (high order) and the active state (low order), perpendicular is the preferred set-up, but sensitive electronics means that any orientation other than parallel to the magnetic field suffices.

However, in yet another embodiment the invention refers to an anisotropic molecule showing a specific dipole moment even in the parallel plane.

In the invention, air is preferably used as the agitating medium. However, it is also possible to have a completely filled cavity if it is ensured that the anisotropic fluid is agitated with body motion (note, it is fluid agitation that results in its altered properties). One such embodiment is a flexible housing completely filled, whereby the motion of the housing provides the agitation. Another embodiment would be to have a completely filled cavity containing inert particles in the fluid, which agitate the fluid with body motion (kind of like the ball bearing in spray-paint cans). If air is the agitator (which is preferred), 98% fluid is a reasonable upper limit. As a lower

limit, enough fluid to fill out the space between electrodes (preferably capacitor plates) is needed, which would necessitate a lower limit of about 20% fluid.

It is important that the sensor is implantable in the human body. For this to be readily made, the sensor is preferably constructed of bio-compatible material. Furthermore, since the housing of the sensor comprises a fluid, it is important that the housing is entirely fluid-tight, in order to secure the function of the sensor as well as the well being of the patient.

The housing may for example consist of glass, ceramic, plexiglass, thermoplastic, curable plastic, metal, rubber (for example silicone rubber) or any other suitable material. Also, the housing may be of any conventional structural biocompatible dielectric material, such as ceramic, phenolic resin, epoxy resin or polysulfone. The shape of the housing may for example be spherical, cylindrical, cubical, of a horse-shoe-shaped annulus form, or any other functional shape.

In one embodiment, the housing is configured in the shape of a cube having six sides, and the electrode includes six generally identical rectangularly shaped side electrodes. Each of these side electrodes is coupled to one side of the housing. The electrodes are electrically accessible outside of the sensor via conventional feed-throughs.

The electrodes can assume different shapes, such as a rectangle, a circle, a triangle, a parabola, or such other geometric shapes that will enable the mapping of the voltages, voltage changes, impedances and impedance changes between various reference points on the side electrodes.

These side electrodes are composed of conventional conductive material such as stainless steel or titanium. The side electrodes may be supported remotely by feed-

through connector wires or may be connected to the side via an insulator.

In still another embodiment the housing comprises means for creating shear forces in the anisotropic fluid by using a solid mechanical moveable element, such as a  
5 bead or a ball made of non-ferromagnetic metal.

The sensitivity of the sensor can be varied by varying the concentration of the anisotropic molecule in the fluid.

10 The sensitivity of the sensor may also be varied by varying the viscosity of the fluid in the housing.

In a second aspect, the invention refers to an electrically detectable anisotropic fluid comprising a liquid crystalline polymer (LCP) as the anisotropic fluid, which LCP is  
15 covalently bound to an iron-oxide nanoparticle. Hereby, a fluid is provided which is specifically adapted for use in a motion sensor of the invention.

In a third aspect, the invention relates to an implantable cardiac pacemaker comprising the implantable motion sensor described above, and means for pacing a  
20 heart, such as a pulse generator, as a response to the activity level as detected by the motion sensor, which means is connected to said motion sensor. The physical activity of the patient in which the pacemaker is implanted is monitored using the sensor, and the output signal of the sensor is used to control the frequency of the pulse generator.

25 In an alternative embodiment of this aspect, the pacemaker does not comprise the motion sensor of the invention, but means for receiving signals from an external motion sensor. In this case, the external motion sensor communicates by means of telemetry or the like with the pacemaker.

By "implantable pacemaker" is meant that the pacemaker in question must be possible to implant in a patient, and thus the pacemaker should be constructed of for example biocompatible material.

5 By "means for pacing a heart" is meant any kind of conventional pacemaker or pulse generator, such as Microny® or implantable cardiac defibrillators comprising such means. The skilled person in the art would know suitable devices for use for this purpose.

10 In one embodiment, the sensor forms an entirely self-contained system within the heart pacemaker, which requires no additional external detectors or line connections outside of the heart pacemaker housing.

In another embodiment, the sensor could be implanted independently, remotely  
15 from the implanted medical device. Yet another alternative would be to have the patient wear the sensor externally, such that the output signals from the sensor are transmitted by telemetry to the implanted medical device.

In any case, the sensor should be as small as possible, e.g. to allow incorporation  
20 into an implantable pacemaker, preferably 0.5 cm square, or less.

In a preferred embodiment the output signal is capacitance, which must first be converted to a voltage signal. The sensor response frequencies need to be calibrated to correspond with appropriate patient motion frequencies.

25 The use of a sensor of the present invention in combination with control circuitry for a heart pacemaker may be as follows (figure 2): The sensor 20 according to this embodiment of the invention comprises a fluid, whose properties of dielectric permittivity change when agitated, causing a corresponding change in the capacitance  
30 between two electrodes (as described above). The variable capacitance is used as an

input signal to 21. 21 is an oscillator, which yields an output frequency that depends on the capacitance input. The frequency generated by 21 is processed and converted to an appropriate signal in 22 (frequency-to-activity-signal conversion), as known in the art. The signal from 22 combined with input of a programmable target rate 31 are further processed in 23 (reaction and recovery circuit) to ensure appropriate reaction time and recovery time of the stimulation to the detected activity signals. The remainder of the flow diagram 24 (pacemaker logic circuit) through 28 are standard and is easily understood by the skilled person in the art of rate-responsive cardiac pacing (25 refers to an output circuit, 26 to an ECG (electrocardiogram) filter and amplifier, 27 to a refractory unit, and 28 to a timer for highest inhibited rate). The total circuit is coupled to the heart 30 of a subject between the output circuit 25 and the ECG filter and amplifier 26. The skilled person in the art would know the various components of the pacemaker circuit. Reference is made to e.g. US-A-5233984 and to Lindgren and Jansson, "Heart Physiology and Stimulation, an introduction", 1992, Siemens-Elma AB, Solna, Sweden.

The control signal for the heart pacemaker may be generated in digital form instead of the analog format discussed above. Digital processing can be undertaken in a microprocessor. In both cases, the programming can be done via a telemetry connection between the heart pacemaker and an external programming means.

In one embodiment of the invention a low/high frequency band pass filter (for measuring a patient's posture and activity) is used. This filter should preferably be calibrated, since the fluid properties of the fluid of the sensor will affect sensor response frequencies. Filtering frequencies may therefore need adjustment.



# Claims:

1. Motion sensor (10, 20) for measuring a patients activity level comprising a fluid-tight, bio-compatible housing (11), a plurality of electrodes (12) being coupled  
5 to the housing, the housing comprising a fluid characterised by that the fluid comprises at least one anisotropic molecule, the anisotropic properties of which are changed in relation to the motion of the fluid, whereby the state of the anisotropic molecules of the fluid is detectable by the electrodes.
2. Motion sensor according to claim 1, which motion sensor is implantable
- 10 3. Motion sensor according to claim 1 or 2, wherein the anisotropic molecule is a liquid crystalline polymer (LCP).
4. Motion sensor according to claim 3, wherein the LCP is poly (p-phenylene) having a degree of polymerisation (n) higher than or equal to 10.
5. Motion sensor according to any one of the preceding claims, whereby the aniso-  
15 tropic molecule comprises an electrically detectable part.
6. Motion sensor according to claim 5, whereby the electrically detectable part is covalently coupled to the anisotropic molecule.
7. Motion sensor according to claim 5 or 6, wherein the electrically detectable part is a magnetic nanoparticle, a zwitterionic pair or a charge separated ion-pair.
- 20 8. Motion sensor according to claim 7, whereby the magnetic nanoparticle is an iron oxide nanoparticle.
9. Motion sensor according to any one of the preceding claims, whereby an external magnetic field (14, 15) is applied to the housing.
10. Motion sensor according to any of the preceding claims, whereby the state of the  
25 anisotropic molecule is monitored by measuring the capacitance in the fluid.
11. Motion sensor according to claim 1-9, whereby the state of the anisotropic molecule is monitored by measuring the resistance in the fluid.
12. Motion sensor according to claim 10, whereby a pair of capacitance electrodes (12, 13) is positioned perpendicular to the applied magnetic field (14, 15).

13. Motion sensor according to any one of claim 1-12, whereby the housing comprises means for creating shear forces in the anisotropic fluid.
14. Electrically detectable anisotropic fluid comprising a liquid crystalline polymer (LCP) as the anisotropic fluid, which LCP is covalently bound to an iron-oxide nanoparticle.
15. Implantable cardiac pacemaker comprising the motion sensor of claim 1-13, or means for receiving signals from an external motion sensor, and means for pacing a heart, as a response to the activity level as detected by the motion sensor, which means for pacing a heart is connected to said motion sensor.

Abstract

The invention relates to an implantable motion sensor for measuring a patient's activity level comprising a fluid-tight, bio-compatible housing, a plurality of electrodes being coupled to the housing, the housing comprising a fluid that the fluid comprises at least one anisotropic molecule, the anisotropic properties of which are changed in relation to the motion of the fluid, whereby the state of the anisotropic molecules of the fluid is detectable by the electrodes. Hereby, the only moving part of the sensor is the anisotropic fluid. Hence, the sensor can be made very small.

Furthermore, the invention relates to an implantable cardiac pacemaker comprising the motion sensor of the invention.

(Fig. 1)

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65  
66  
67  
68  
69  
70  
71  
72  
73  
74  
75  
76  
77  
78  
79  
80  
81  
82  
83  
84  
85  
86  
87  
88  
89  
90  
91  
92  
93  
94  
95  
96  
97  
98  
99  
100  
101  
102  
103  
104  
105  
106  
107  
108  
109  
110  
111  
112  
113  
114  
115  
116  
117  
118  
119  
120  
121  
122  
123  
124  
125  
126  
127  
128  
129  
130  
131  
132  
133  
134  
135  
136  
137  
138  
139  
140  
141  
142  
143  
144  
145  
146  
147  
148  
149  
150  
151  
152  
153  
154  
155  
156  
157  
158  
159  
160  
161  
162  
163  
164  
165  
166  
167  
168  
169  
170  
171  
172  
173  
174  
175  
176  
177  
178  
179  
180  
181  
182  
183  
184  
185  
186  
187  
188  
189  
190  
191  
192  
193  
194  
195  
196  
197  
198  
199  
200  
201  
202  
203  
204  
205  
206  
207  
208  
209  
210  
211  
212  
213  
214  
215  
216  
217  
218  
219  
220  
221  
222  
223  
224  
225  
226  
227  
228  
229  
230  
231  
232  
233  
234  
235  
236  
237  
238  
239  
240  
241  
242  
243  
244  
245  
246  
247  
248  
249  
250  
251  
252  
253  
254  
255  
256  
257  
258  
259  
260  
261  
262  
263  
264  
265  
266  
267  
268  
269  
270  
271  
272  
273  
274  
275  
276  
277  
278  
279  
280  
281  
282  
283  
284  
285  
286  
287  
288  
289  
290  
291  
292  
293  
294  
295  
296  
297  
298  
299  
300  
301  
302  
303  
304  
305  
306  
307  
308  
309  
310  
311  
312  
313  
314  
315  
316  
317  
318  
319  
320  
321  
322  
323  
324  
325  
326  
327  
328  
329  
330  
331  
332  
333  
334  
335  
336  
337  
338  
339  
340  
341  
342  
343  
344  
345  
346  
347  
348  
349  
350  
351  
352  
353  
354  
355  
356  
357  
358  
359  
360  
361  
362  
363  
364  
365  
366  
367  
368  
369  
370  
371  
372  
373  
374  
375  
376  
377  
378  
379  
380  
381  
382  
383  
384  
385  
386  
387  
388  
389  
390  
391  
392  
393  
394  
395  
396  
397  
398  
399  
400  
401  
402  
403  
404  
405  
406  
407  
408  
409  
410  
411  
412  
413  
414  
415  
416  
417  
418  
419  
420  
421  
422  
423  
424  
425  
426  
427  
428  
429  
430  
431  
432  
433  
434  
435  
436  
437  
438  
439  
440  
441  
442  
443  
444  
445  
446  
447  
448  
449  
450  
451  
452  
453  
454  
455  
456  
457  
458  
459  
460  
461  
462  
463  
464  
465  
466  
467  
468  
469  
470  
471  
472  
473  
474  
475  
476  
477  
478  
479  
480  
481  
482  
483  
484  
485  
486  
487  
488  
489  
490  
491  
492  
493  
494  
495  
496  
497  
498  
499  
500  
501  
502  
503  
504  
505  
506  
507  
508  
509  
510  
511  
512  
513  
514  
515  
516  
517  
518  
519  
520  
521  
522  
523  
524  
525  
526  
527  
528  
529  
530  
531  
532  
533  
534  
535  
536  
537  
538  
539  
540  
541  
542  
543  
544  
545  
546  
547  
548  
549  
550  
551  
552  
553  
554  
555  
556  
557  
558  
559  
560  
561  
562  
563  
564  
565  
566  
567  
568  
569  
570  
571  
572  
573  
574  
575  
576  
577  
578  
579  
580  
581  
582  
583  
584  
585  
586  
587  
588  
589  
590  
591  
592  
593  
594  
595  
596  
597  
598  
599  
600  
601  
602  
603  
604  
605  
606  
607  
608  
609  
610  
611  
612  
613  
614  
615  
616  
617  
618  
619  
620  
621  
622  
623  
624  
625  
626  
627  
628  
629  
630  
631  
632  
633  
634  
635  
636  
637  
638  
639  
640  
641  
642  
643  
644  
645  
646  
647  
648  
649  
650  
651  
652  
653  
654  
655  
656  
657  
658  
659  
660  
661  
662  
663  
664  
665  
666  
667  
668  
669  
670  
671  
672  
673  
674  
675  
676  
677  
678  
679  
680  
681  
682  
683  
684  
685  
686  
687  
688  
689  
690  
691  
692  
693  
694  
695  
696  
697  
698  
699  
700  
701  
702  
703  
704  
705  
706  
707  
708  
709  
710  
711  
712  
713  
714  
715  
716  
717  
718  
719  
720  
721  
722  
723  
724  
725  
726  
727  
728  
729  
730  
731  
732  
733  
734  
735  
736  
737  
738  
739  
740  
741  
742  
743  
744  
745  
746  
747  
748  
749  
750  
751  
752  
753  
754  
755  
756  
757  
758  
759  
760  
761  
762  
763  
764  
765  
766  
767  
768  
769  
770  
771  
772  
773  
774  
775  
776  
777  
778  
779  
780  
781  
782  
783  
784  
785  
786  
787  
788  
789  
790  
791  
792  
793  
794  
795  
796  
797  
798  
799  
800  
801  
802  
803  
804  
805  
806  
807  
808  
809  
810  
811  
812  
813  
814  
815  
816  
817  
818  
819  
820  
821  
822  
823  
824  
825  
826  
827  
828  
829  
830  
831  
832  
833  
834  
835  
836  
837  
838  
839  
840  
841  
842  
843  
844  
845  
846  
847  
848  
849  
850  
851  
852  
853  
854  
855  
856  
857  
858  
859  
860  
861  
862  
863  
864  
865  
866  
867  
868  
869  
870  
871  
872  
873  
874  
875  
876  
877  
878  
879  
880  
881  
882  
883  
884  
885  
886  
887  
888  
889  
890  
891  
892  
893  
894  
895  
896  
897  
898  
899  
900  
901  
902  
903  
904  
905  
906  
907  
908  
909  
910  
911  
912  
913  
914  
915  
916  
917  
918  
919  
920  
921  
922  
923  
924  
925  
926  
927  
928  
929  
930  
931  
932  
933  
934  
935  
936  
937  
938  
939  
940  
941  
942  
943  
944  
945  
946  
947  
948  
949  
950  
951  
952  
953  
954  
955  
956  
957  
958  
959  
960  
961  
962  
963  
964  
965  
966  
967  
968  
969  
970  
971  
972  
973  
974  
975  
976  
977  
978  
979  
980  
981  
982  
983  
984  
985  
986  
987  
988  
989  
990  
991  
992  
993  
994  
995  
996  
997  
998  
999  
1000

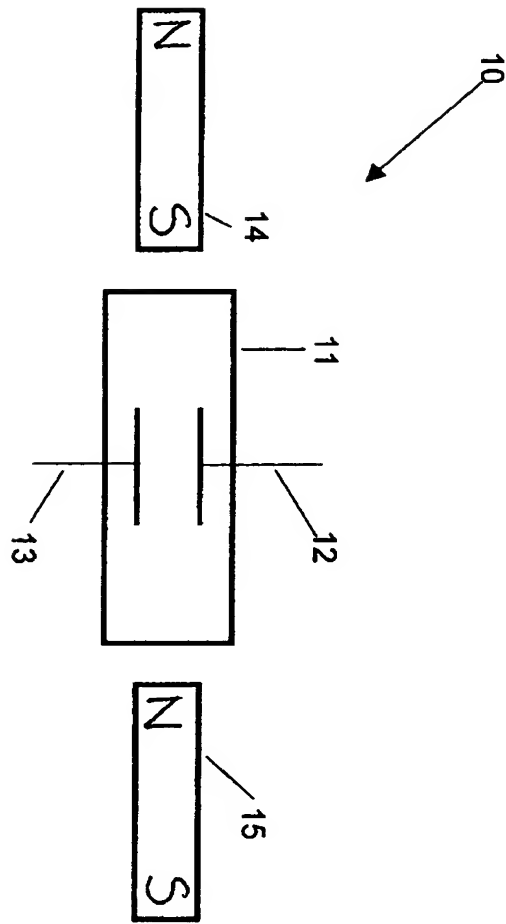


Fig. 1

6-0000000000

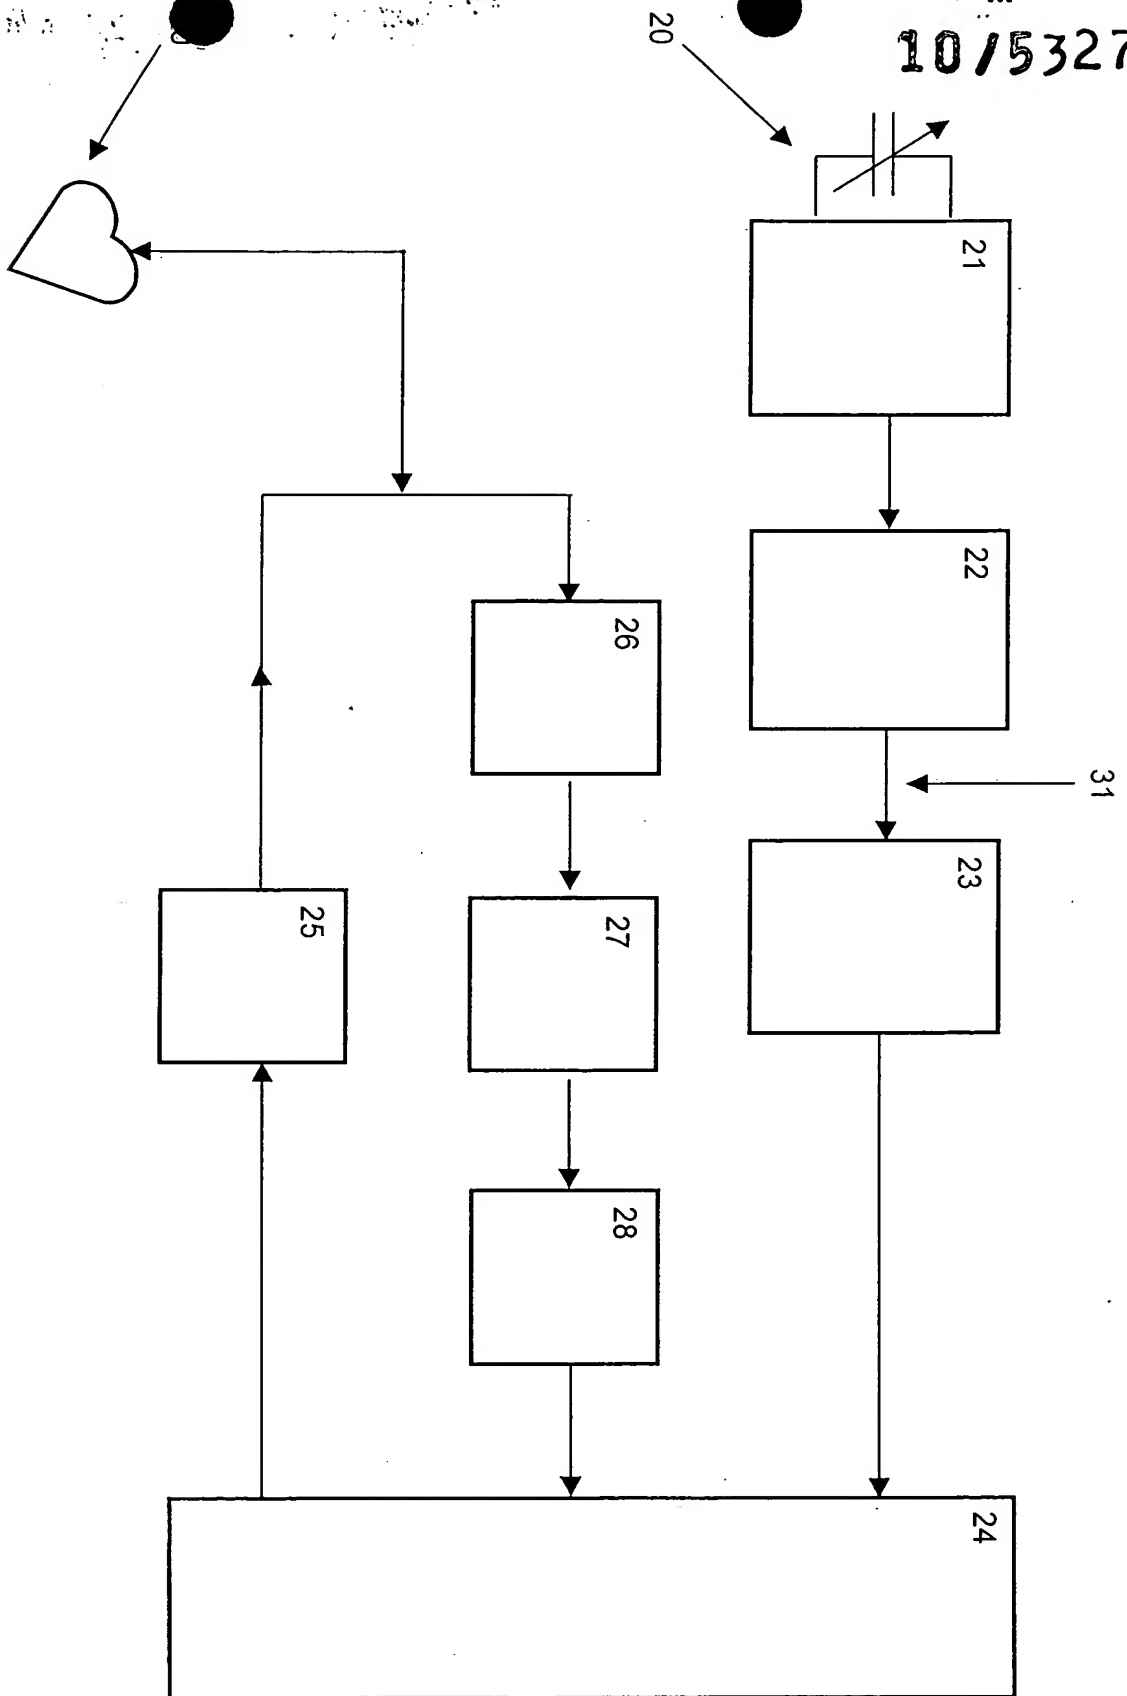


Fig. 2